


stryker

AlphaVent Knotless

Self-punching, knotless anchor platform

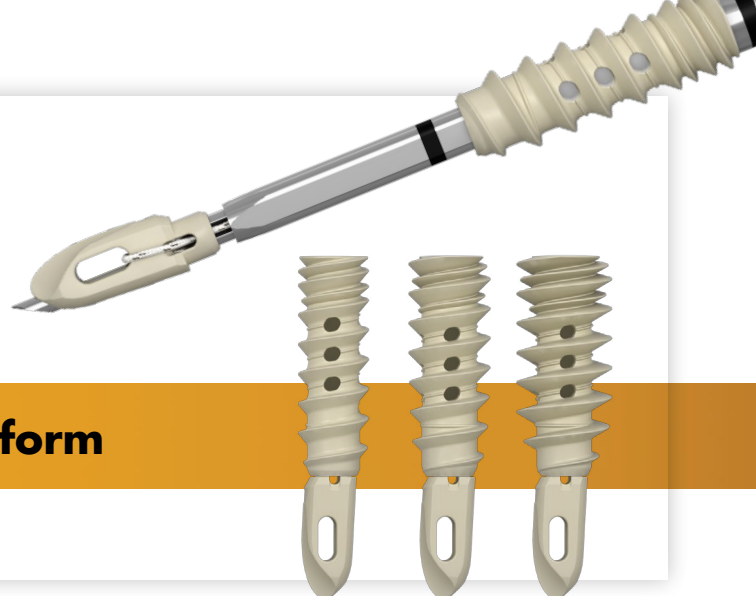

4.75mm 5.5mm 6.5mm

Streamlined design




Coupled, self-punching anchor system

Alleviates need for pilot hole creation*

Coupled eyelet and anchor facilitate streamlined tensioning


*Pilot hole creation required for hard bone indications.

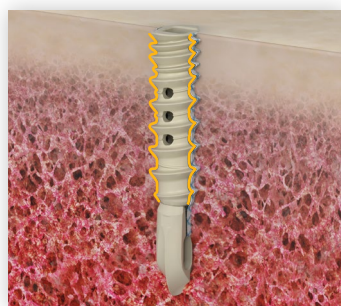

Dual-thread Technology

Devised to improve anchor performance through optimized engagement in cortical and cancellous bone¹

Provides tactile feedback during cortical thread engagement¹

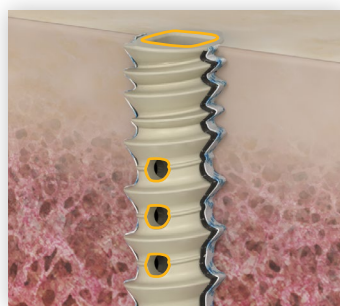

Complete venting and cannulation

Allows exchange of blood and other autologous cells at the healing site




Your repair. Your way.

Accommodates a variety of suture configurations

Anchor length enables use in a single and double row repair

Features

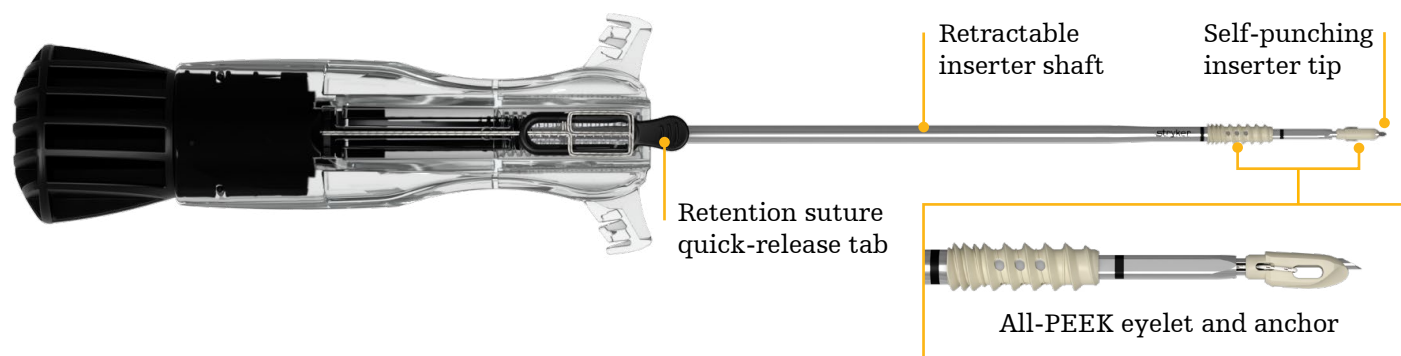

Hard bone instrumentation



3.9mm Omega and 4.75mm AlphaVent awl



4.75mm AlphaVent and Omega awl



4.75mm AlphaVent punch-tap



4.75mm AlphaVent tap



5.5mm AlphaVent tap



Drill guide



4.75mm AlphaVent and Omega drill



5.5mm AlphaVent and 4.75mm hard bone Omega drill

AlphaVent Knotless offerings

Implants

3910956547	AlphaVent Knotless SP, 4.75mm PEEK anchor
3910956555	AlphaVent Knotless SP, 5.5mm PEEK anchor
3910956565	AlphaVent Knotless SP, 6.5mm PEEK anchor

Instrumentation

3910947200	3.9mm Omega and 4.75mm AlphaVent awl
3910947201	4.75mm AlphaVent and Omega awl
3910947202	4.75mm AlphaVent and Omega drill
3910947207	4.75mm AlphaVent tap
3910947208	4.75mm AlphaVent punch-tap
3910947203	5.5mm AlphaVent and 4.75mm hard bone Omega drill
3910947209	5.5mm AlphaVent tap
3910947212	Drill guide

References:

1. TR22963

Sports Medicine

This document is intended solely for the use of healthcare professionals. A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. We do not dispense medical advice and recommend that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate Stryker's products. A surgeon must always refer to the package insert, product label and/or instructions for use, including the instructions for cleaning and sterilization (if applicable), before using any of Stryker's products. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets.

Please contact your representative if you have questions about the availability of Stryker's products in your area.

Stryker or its affiliated entities own, use, or have applied for the following trademarks or service marks: AlphaVent, Omega and Stryker. All other trademarks are trademarks of their respective owners or holders.

The absence of a product, feature, or service name, or logo from this list does not constitute a waiver of Stryker's trademark or other intellectual property rights concerning that name or logo.

1000904690 Rev A

Copyright © 2024 Stryker

Stryker
Sports Medicine
5670 Greenwood Plaza Blvd.
Ste. 200
Greenwood Village, CO 80111
t: 866 596 2022
www.sportsmedicine.stryker.com